

ULTRASONIC THERAPEUTIC DEVICE FOOT SWITCH I/F CIRCUIT O POWER AMPLIFIER /24 20 D/A CONTROL CIRCUIT 726 OSCILLATING CIRCUIT 121 PANEL

16 *q9-*⇔ 39~ 41a 51a 43 6á 45 (Ö) 31 52 410 41f 41e 41b 53 50 55

FIG.4

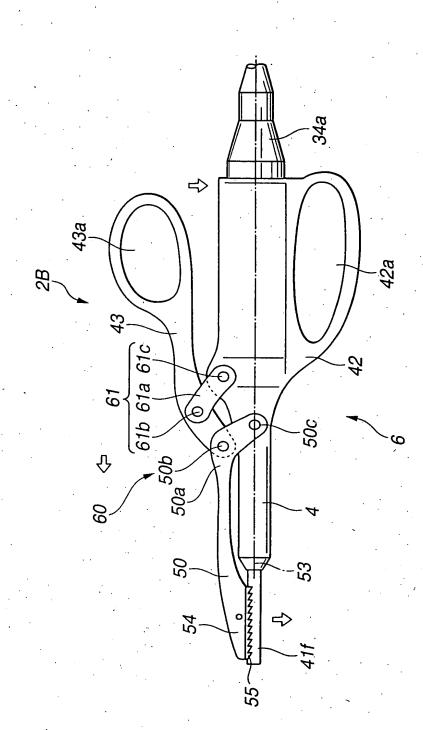


FIG.6

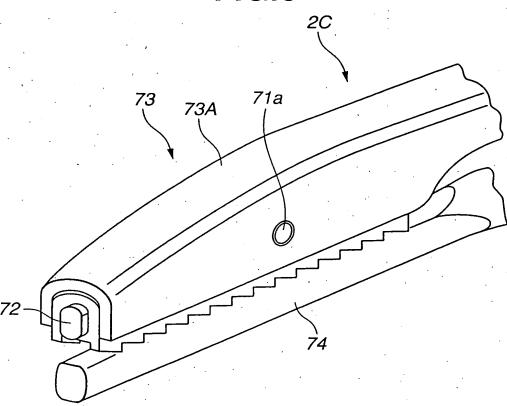


FIG.9

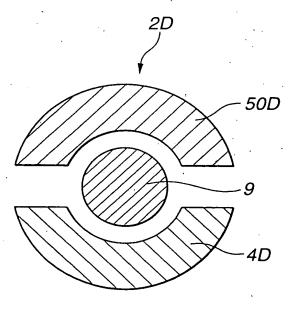
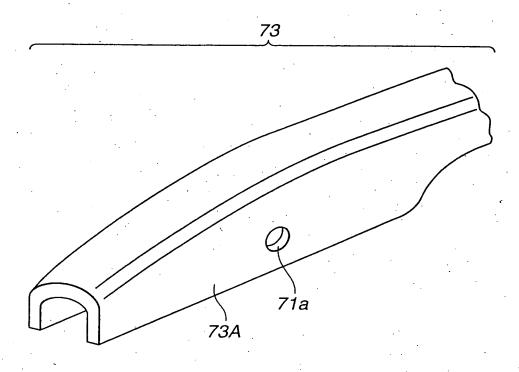


FIG.7



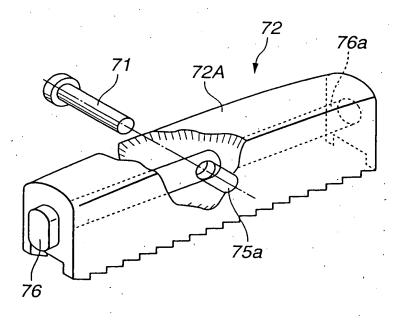


FIG.8

34a 34 43a ф 62 4E 41f(9) 54

FIG.10